


Agitator for tissue Ext.Diam. 60 mm (without stirring motor) | N4300

Compliant with standards

NFQ 34.020; ISO 12625-17



Description

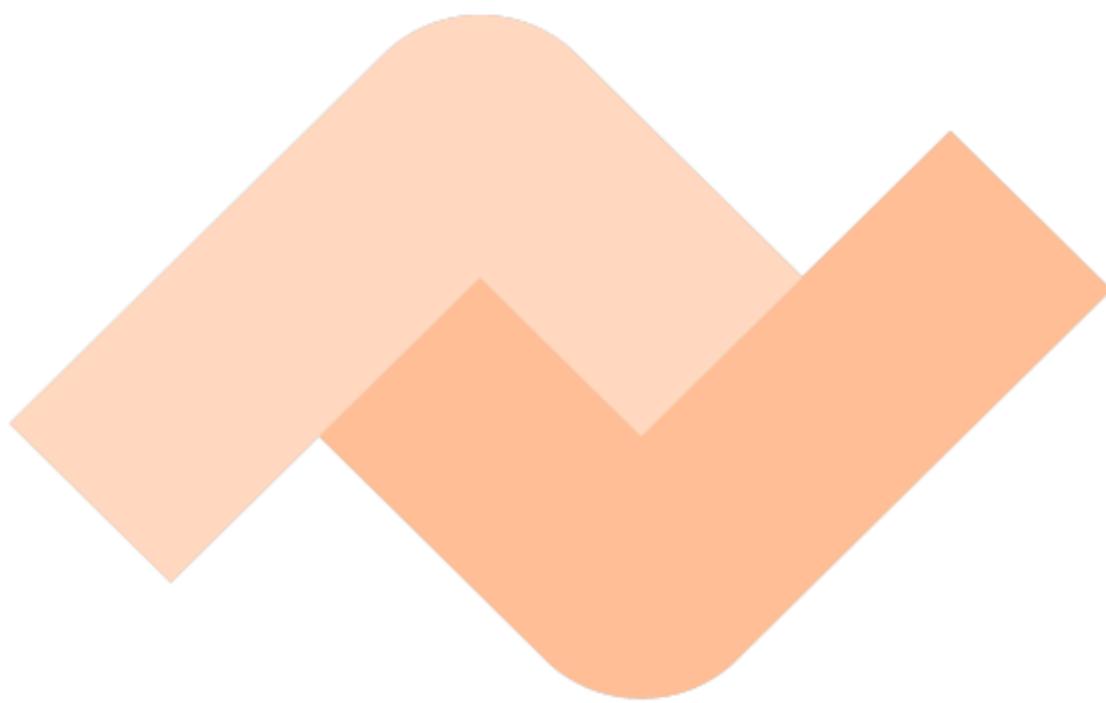

Sold & serviced by:

OpTest Equipment Inc.

www.optest.com - sales@optest.com - +1-613-632-5169